BK Medical

# Product Catalog

2011-10-12 / BG0143-Z

BK Medical

## Trademarks

Adobe®
CIDEX®
CIV-Flex™
DICOM®
IQPAC™
Magnum®
Microsoft®
Micro-Touch®
NeoGuard®
Storz®
Welch Allyn®

BK Medical

# Table of Contents


**Systems ..... 1**
Pro Focus 2202 System ..... 1
Available versions for Pro Focus ..... 1
Flex Focus 1202 System ..... 1
Available versions for Flex Focus ..... 1
2202 Upgrade Options ..... 3

**Accessories for Pro Focus 2202 ..... 7**
PCU ..... 7
Trackball Adjustment Tool ..... 7
Foot Switch ..... 7
Hand Rest for 2202 ..... 7
Foot Switch ..... 7
Cord Retaining Kit ..... 7
Network Isolator ..... 7
Transducer Holder Inlay ..... 7
Extension Cable for Front Panel ..... 7
Endo Transducer Holder for Pro Focus ..... 8
Transducer Holder for Transducer 8838 for use on Pro Focus 2202 UltraView. ..... 8
Shortcut Stickers for Pro Focus ..... 8
System Cover ..... 8
Flight Case for 2202 ..... 8
Digital B/W Printer Start-Up Kit ..... 8
Printer Shelf ..... 8
SONY Monitor ..... 8

**Accessories for Flex Focus 1202 ..... 9**
Power Pack ..... 9
Battery Charger Station ..... 9
Mobile Keyboard Dock ..... 9
Keyboard Wall Dock ..... 9
Mobile Keyboard Dock ..... 9
Keyboard Table Dock ..... 9
Mobile Touch Dock ..... 9
Touch Wall Dock ..... 9
Mobile Touch Dock ..... 10
Backpack for Flex Focus ..... 10
DVD Drive (upgrade) ..... 10
Remote Control ..... 10
Wheeled Transport Case ..... 10
Endo Transducer Holder ..... 10
Endo Transducer Holder Mount ..... 10
Wall-Mounted Transducer Holder ..... 10
Transducer Connector to mount on the wall (dummy) 10
Foot Switch ..... 11
Video Cable (Flex Focus to phono and BNC) ..... 11
Transducer Holder ..... 11

**3D Imaging Accessories for Pro Focus 2202 and Flex Focus 1202 ..... 12**
Magnetic Wheel Mover ..... 12
Adapter Ring for 8848 ..... 12
Adapter Ring for 8808 ..... 12
Adapter Ring for 8818/8808e ..... 12
Pullback Adapter for 8848 ..... 12
Pullback Adapter for 8818/8808e ..... 12
Adapter Cable for 1202 ..... 12
Variable Friction Support Arm ..... 12
Foot Switch ..... 12
Foot Switch ..... 12
3D Connector Box ..... 12

**Documentation Accessories ..... 13**
Printing Paper SONY UPP-110HA ..... 13
Printing Paper SONY UPP-110HG ..... 13
Color Printing Pack SONY UPC-21S ..... 13
Digital B/W Printer SONY UP-D897 ..... 13
Digital B/W Printer SONY UP-D897 for Flex Focus 1202 ..... 13
Digital Color Printer SONY UP-D25MD for Pro Focus 2202 UltraView ..... 13
Printer Start-Up Kit for Flex Focus 1202 ..... 13

**Power Cables ..... 14**

**Miscellaneous ..... 18**
Scanning Gel ..... 18
OB Stickers for keyboard shortcuts ..... 18
Breast Ultrasound Biopsy Phantom. Model 052 ..... 18
Tissue Equivalent Ultrasound Prostate Phantom Model 053 ..... 18
Biplane Prostate Phantom ..... 18
Endfire Prostate Phantom ..... 18

**Transducers and Transducer Accessories ..... 19**
Endosonic Transducer 1850-M ..... 19
Endosonic Transducer 1850-M (continued) ..... 20
Anorectal Transducers 2050 and 2052 ..... 21

# Table of Contents


Mechanical Sector Transducer 8551-R ..... 22
Laparoscopic Transducer 8666-RF ..... 22
Convex Array Transducer 8667 ..... 23
Linear Array Transducer 8670 ..... 23
Convex Array Transducer 8802 ..... 24
Biplane Transducer 8808 ..... 25
Endorectal Biplane Transducer 8808e ..... 26
Linear Array Transducer 8809 ..... 27
Linear Array Transducer 8811 ..... 27
Linear Array Transducer 8812 ..... 28
Intraoperative Transducer 8814 ..... 28
Intraoperative Transducer 8815 ..... 29
T-Shaped Intraoperative Transducer 8816 ..... 29
Biplane and Endfire Transducer 8818 ..... 30
Endovaginal Endfire Transducer 8819 ..... 31
Convex Array Transducer 8820e ..... 31
Vascular Transducer 8822 ..... 32
Convex Array Transducer 8823 ..... 32
I and T Shaped Intraoperative Transducer 8824 ..... 33
ProART Robotic Transducer 8826 ..... 33
Convex Array Transducer 8830 ..... 34
3DART Transducer 8838 ..... 35
Transducer 8848 ..... 36
Craniotomy Transducer 8862 ..... 36
Burr Hole Transducer 8863 ..... 37
High Frequency Linear Array Transducer 8870 ..... 37
CIVCO AccuCare Stepper Units (Barzell-Whitmore) ..... 38

# Systems

**2202**

## Pro Focus 2202 System

Printer must be ordered separately.

### Available versions for Pro Focus

**2202-7-UltraView** — High-End Color System

**2202-2-Green (C)** — Midrange Color System

**2202-9-OR** — Pro Focus UltraView OR

**1202**

## Flex Focus 1202 System

Keyboard Dock, printer etc. must be ordered separately.

### Available versions for Flex Focus

**1202-3**
Flex Focus 700
Dedicated to surgery.

**1202-1**
Flex Focus 400
Color system with IQPAC™.

**1202-4**
Flex Focus 400 Anesthesia
Dedicated to regional anesthesia.

**1202-2**
Flex Focus 200
Flex Focus with basic functionality. B&W system. Upgradable to color.

**1202-7**
Flex Focus 200 Surgery
Basic surgical system with limited transducer range.

| Available versions of Pro Focus 2202 | | |
|---|---|---|
| **Part no. Pre-order** | **Feature** | **UltraView 2202-7** |
| | IQPAC™ | Included |
| | Color Flow Mapping | Included |
| | Power Doppler | Included |
| | Directional Power Doppler | Included |
| | Pulsed Wave Doppler | Included |
| | Continuous Wave Doppler | Included |
| UA2214 | Tissue Harmonic Imaging | Included |
| UA2215 | Contrast Imaging (License)[1] | Optional |
| UA2206 | DICOM Option (License) | Optional |
| UA1205 | Picture-in-Picture | Optional |
| UA2238 | HistoScanning™ Interface Option for 2202 UltraView[2] | Optional |
| UA2238-K | HistoScanning™ Interface Upgrade Kit for 2202 UltraView[2] | Optional |
| UA2235 | HistoScanning™ Interface Option for 2202 Yellow (CX)[2] | NA |
| UA2235-K | HistoScanning™ Interface Upgrade Kit for 2202 Yellow (CX)[2] | NA |
| UA2236 | HistoScanning™ Interface Option for 2202 Green (C)[2] | NA |
| UA2236-K | HistoScanning™ Interface Upgrade Kit for 2202 Green (C)[2] | NA |
| UA2237-K | HistoScanning™ Interface Upgrade Kit for 2202 Yellow (CX) and Green (C)[2] | NA |
| UA2226 | Varian Option License | Optional |
| UA2226-K | Varian Option Upgrade Kit | Optional |
| UA2207 | 3D Freehand (License) | Optional |
| UA2222 | 3D Professional (includes 3D Mover Module and Freehand) | Optional |
| UA2222-K | 3D Mover Module Kit (from Freehand to Professional. Must be ordered with UA2207) | Optional |
| UA2223 | 360° Mechanical Input Module | Optional |
| UA2223-K | 360° Mechanical Input Module Kit (Upgrade) | Optional |
| UA2251 | Flat Screen for 2202 | NA |
| UA2251-K | Flat Screen Kit for 2202 | NA |
| UA2252 | Flat Screen on Arm for 2202 | NA |
| UA2252-K | Flat Screen on Arm Kit for 2202 | NA |
| | Height-Adjustable Keyboard Panel and Monitor (Simultaneous Movement) | Included |
| | Height-Adjustable Keyboard Panel and Monitor (Independent Movement) | NA |
| UA2220 | 3rd Linear and Convex Array (Electronic) Transducer Connector Active | Included |

# Systems

| Available versions of Pro Focus 2202 | | |
|---|---|---|
| **Part no. Pre-order** | **Feature** | **UltraView 2202-7** |
| | Support for transducers: 8667, 8670, 8802, 8808, 8809, 8811, 8818, 8819, 8820e, 8823, 8827, 8848 | Included |
| | Support for transducers: 8666-RF, 8808e, 8812, 8814, 8815, 8816, 8822, 8824, 8826, 8838, 8862, 8863, 8870 | Included |
| | Support for Single Element (Mechanical) transducers: 1850, 2050, 2052, 8551[3] | Optional |
| UA2410 | Palm Control Unit (PCU). See page 7 for more details. | Optional |
| UA4100 | Digital B/W Printer Start-Up Kit. See page 8 for more details. | Optional |

1 In the USA, contrast-enhanced ultrasound has not been market cleared by the FDA, with the exception of only select cardiac applications.
2 HistoScanning has not been market cleared by the FDA for sale in the USA.
3 Transducer Type 8551 is not supported on UltraView.

## 2202 Upgrade Options

**UA2233-K** B/W to Color Upgrade Kit†

**UA2229-K** Transducer Support Upgrade Kit

Required to support 8818 on systems from before March 2006 and to support 8848 on systems from before January 2007. Contact Service for further details.

† For systems purchased after February 2007.

| Options for Flex Focus 1202 | | | | | | |
|---|---|---|---|---|---|---|
| **Part no. Pre-order** | **• Included ° Optional Feature** | **Flex Focus 200** | **Flex Focus 200 Surgery** | **Flex Focus 400** | **Flex Focus 400 Anesthe-sia** | **Flex Focus 700** |
| UA1210 | Mobile Keyboard Dock | ° | ° | ° | ° | ° |
| UA1214 | Mobile Keyboard Dock with battery (includes 2 rechargable batteries) | ° | ° | ° | ° | ° |
| UA1211 | Keyboard Wall Dock | ° | ° | ° | ° | ° |
| UA1283 | Keyboard Table Dock | ° | ° | ° | ° | ° |
| UA1810 | Mobile Touch Dock | ° | ° | ° | ° | ° |
| UA1811 | Touch Wall Dock (no DVD [RW]) | ° | ° | ° | ° | ° |
| UA1814 | Mobile Touch Dock with battery (includes 2 rechargable batteries) | ° | ° | ° | ° | ° |
| UA1222 | 3D Professional (License) - includes 3D Freehand | NA | NA | ° | NA | ° |
| UA1207 | 3D Freehand (License) | NA | NA | ° | ° | ° |
| UA1206 | DICOM (License) | ° | ° | ° | ° | ° |
| UA1226 | Varian Option (License) | NA | NA | ° | NA | ° |
| UA1203 | Color Doppler (Color Flow Mapping) | 1 | ° | • | • | • |
| UA1298 | Pulsed Wave Dopple (PW) | 1 | ° | • | • | • |
| UA1205 | Picture-in-Picture | NA | NA | NA | NA | ° |
| | IQPAC™ | NA | NA | • | • | • |
| | Clip Store | NA | NA | • | • | • |
| | Video Out | NA | • | • | • | • |
| | Basic Transducer Support: 8667, 8670, 8808, 8808e, 8811, 8819, 8820e, 8823, 8827, 8830 | • | • | • | NA | • |
| | Enhanced Transducer Support: 1850, 2050, 2052, 8802, 8809, 8818, 8822, 8838, 8848, 8862, 8863, 8870 | NA | NA | • | NA | • |
| | Anesthesia Transducer Support: 8670, 8809, 8811, 8816, 8823, 8827, 8830, 8870 | NA | NA | NA | • | NA |
| UA1258 | Basic Surgical Transducer Support: 8666-RF, 8815, 8816 | NA | • | NA | NA | NA |
| | Complete Surgical Transducer Support (all transducers) | NA | NA | NA | NA | • |
| UA1237 | Remote Control for Flex Focus 700 (includes Mini Bluetooth Adapter) | NA | NA | NA | NA | ° |
| UA1294 | Endo Transducer Holder | NA | ° | ° | NA | ° |
| UA1295 | Endo Transducer Holder Mount (for UA1294 with 1850 or 2052) | NA | ° | ° | NA | ° |
| UA1204 | Wall-Mounted Transducer Holder | ° | ° | ° | ° | ° |

| Options for Flex Focus 1202 | | | | | | |
|---|---|---|---|---|---|---|
| **Part no. Pre-order** | **• Included ° Optional<br>Feature** | **Flex Focus 200** | **Flex Focus 200 Surgery** | **Flex Focus 400** | **Flex Focus 400 Anesthe-sia** | **Flex Focus 700** |
| UA1296 | General Transducer Holder (requires UA1810 or UA1814) | ° | ° | ° | ° | ° |
| UA1223 | Power Cable Holder. Included with UA1214 and UA1814 | ° | ° | ° | ° | ° |
| UA1220 | Backpack to hold printer. Requires Mobile Dock UA1210 | ° | ° | ° | ° | ° |
| UA1202 | Foot Switch (USB) | ° | ° | ° | ° | ° |
| UA1284-K | DVD RW Drive Kit | ° | ° | ° | ° | NA |
| UA1247 | Battery Charger Station[1] | ° | ° | ° | ° | ° |
| UA1225 | Extra Battery for UA 1214 and UA1814 (rechargable 14.4 V lithium ion battery). Must be ordered in sets of 2 or 4 batteries. | ° | ° | ° | ° | ° |
| QA0228 | Trackball Adjustment Tool | • | • | • | • | NA |
| UA4102 | Printer Start-Up Kit. Requires UA1220, UA1214 or UA1814 | ° | ° | ° | ° | ° |
| AO0491 | Video Cable (Flex Focus to phono and BNC) | ° | ° | ° | ° | NA |
| UA0964 | Flight Case - for scanner unit with Mobile Keyboard Dock | ° | ° | ° | ° | ° |
| UA1285 | Wheeled Transport Case - suitcase on wheels for scanner unit without dock, plus two transducers. | ° | ° | ° | ° | ° |

1 Only available in some countries.

# *flex* Focus

## Flexibility concept

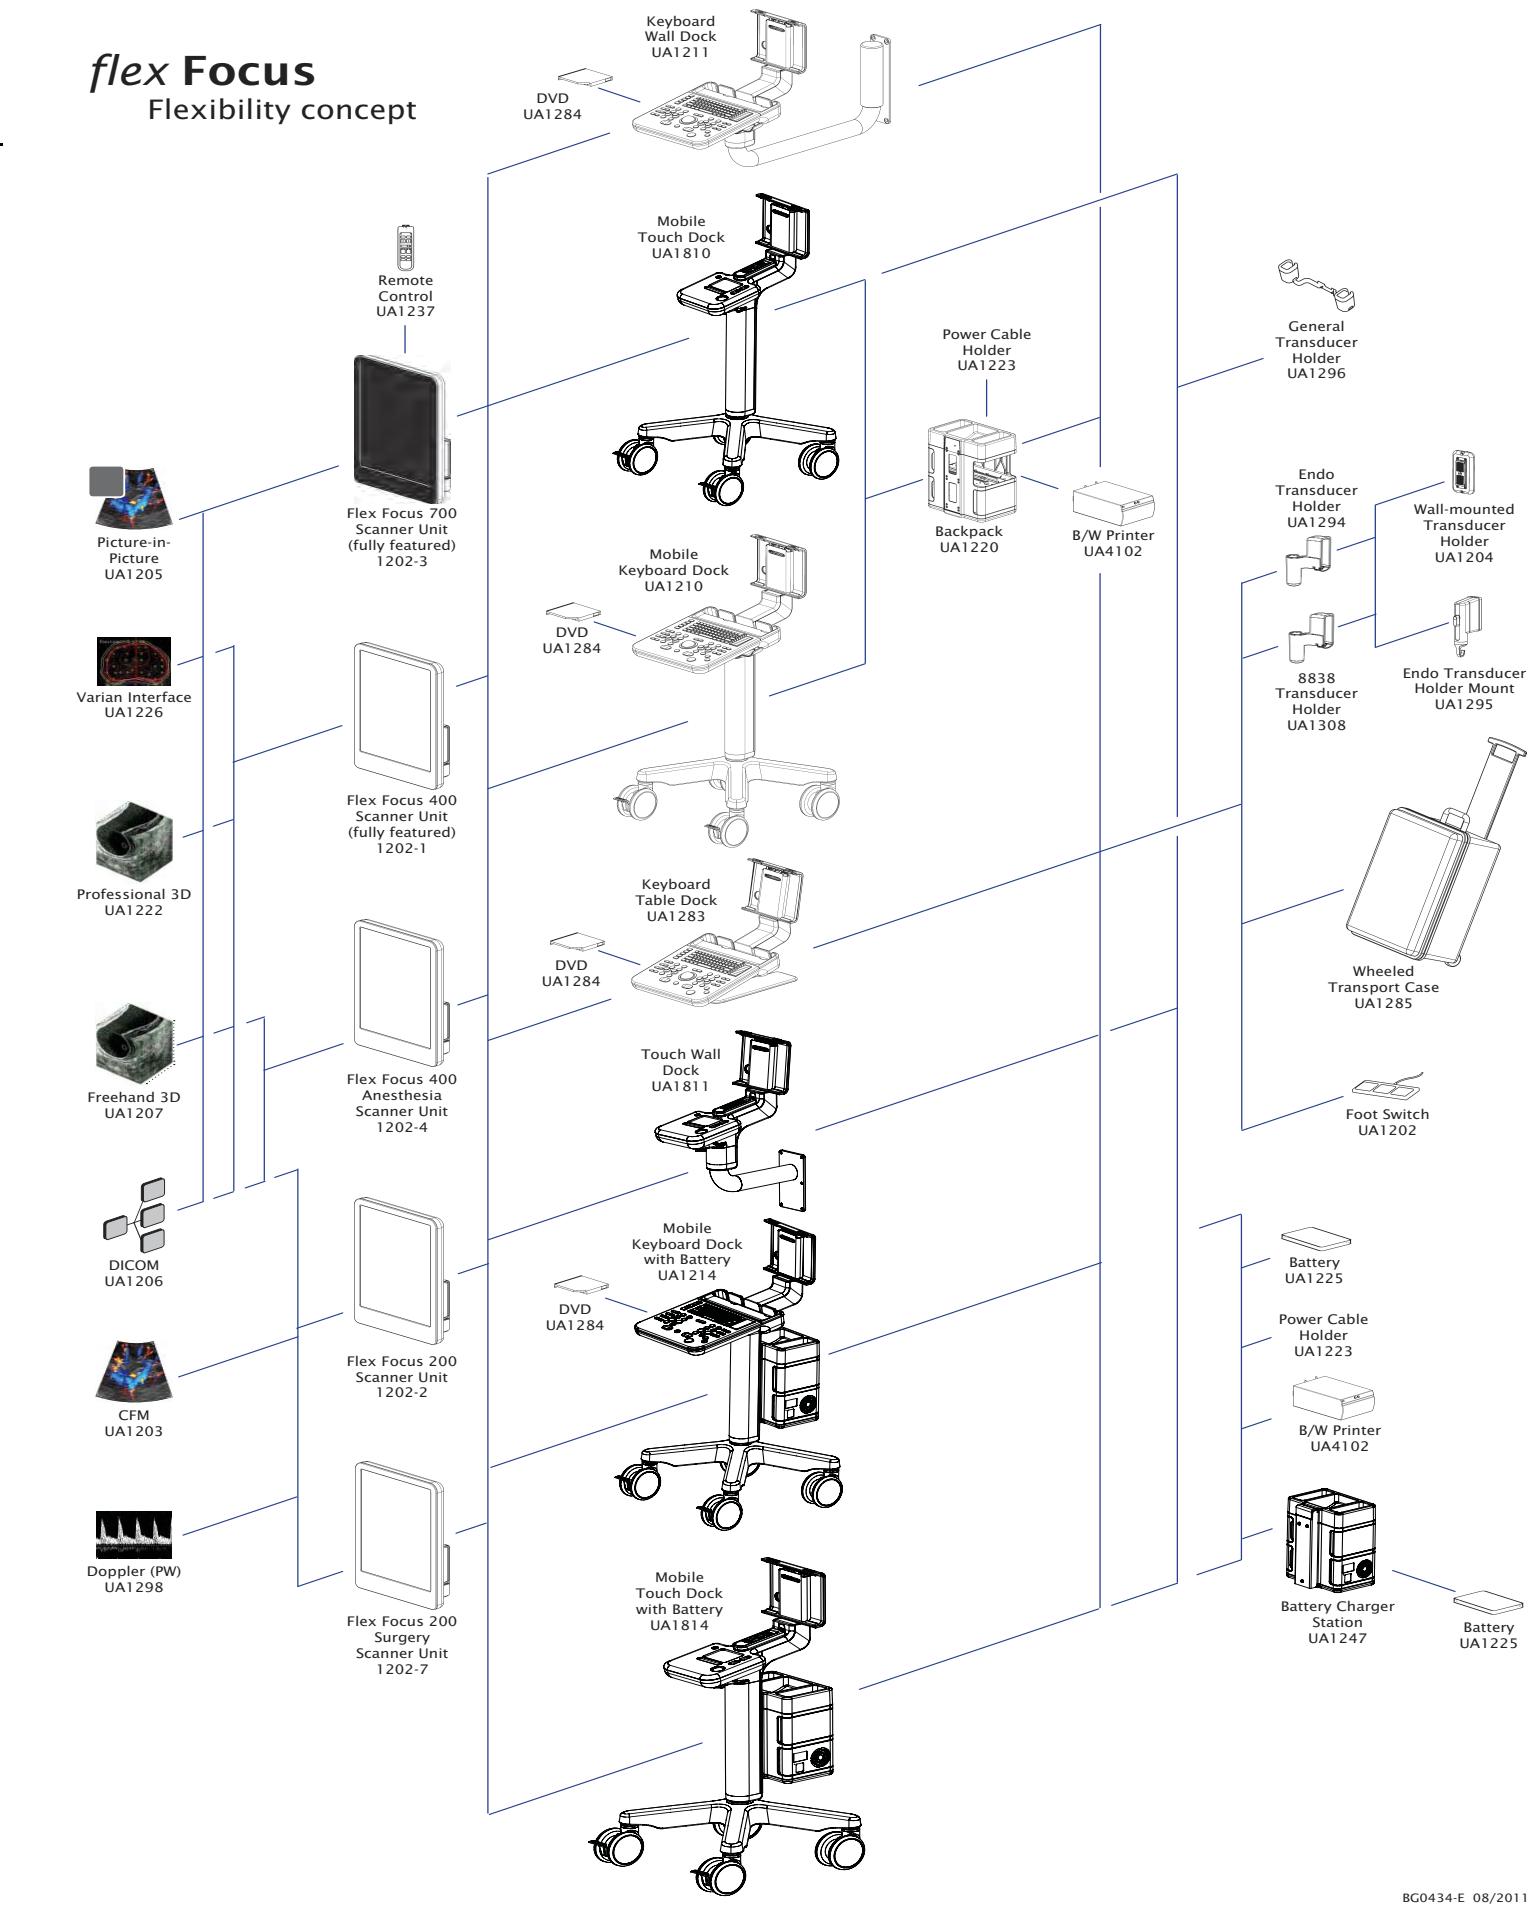


BG0434-E 08/2011

# Accessories for Pro Focus 2202

**UA2410**

**PCU**

Palm Control Unit for 2202. Allows the user to operate all major functions remotely. The Palm Control Unit may be disinfected and sterilized.
Ideal for the surgical environment.

**UA1271**

Adapter for PCU. Needed to connect UA2410 to 2202.

**UA0076**

Sterile cover, 14 x 147 cm, latex-free

**QA0228**



**Trackball Adjustment Tool**

Tool to adjust the trackball tension on 2202 and 1202.

Included with the system.

**UA1215**

**Foot Switch**

2-pedal high-quality foot switch. Both pedals are user-configurable when connected to 2202 Yellow, Green or Blue.

**DS0967**

**Hand Rest for 2202**

The removable hand rest can be used to make working with the keyboard panel more comfortable.

**UA1202**

**Foot Switch**

For Pro Focus 2202 Ultraview and Flex Focus 1202.

## Cables and Connectors

**UA2204**

**Cord Retaining Kit**

**DP0925**

**Network Isolator**

**DZ9756**

**Transducer Holder Inlay**

Inlay for the transducer holders on the system. This allows very small transducers, such as the 8809, to be securely stored on the system.
Only if extras are needed. 1 is included as standard with the transducer.

**AO0421**



**Extension Cable for Front Panel**

Unique BK Medical feature.
Using the extension cable, the system can be operated from up to 3 meters away.

# Accessories for Pro Focus 2202

**UA1302**

**Endo Transducer Holder for Pro Focus**

Holds all large endo transducers and the ECRM-Mover in a stable position when not in use.

**UA1347**



**Transducer Holder for Transducer 8838 for use on Pro Focus 2202 UltraView.**

**SC1624**

**Shortcut Stickers for Pro Focus**

**UA0955**

**System Cover**

**UA0959**

**Flight Case for 2202**

**UA4100**

**Digital B/W Printer Start-Up Kit**

Must be orderede separately. Consists of a SONY UP-D897 printer, a USB cable, a power cable and 10 rolls of printer paper.

**UA2240**

**Printer Shelf**

**SONY Monitor**

SONY LMD214OMD medical grade LCD monitor.

# Accessories for Flex Focus 1202

## Flex Focus Scanner Units

**1201-1, 2, 4 or 7**

1202-1 (Flex Focus 400) is a color scanner unit. The 1202-2 (Flex Focus 200) is a Flex Focus scanner unit, with basic funtionality and 1202-4 (Flex Focus 400 Anesthesia) is dedicated to regional anesthesia. A Flex Focus 200 system or 400 Anesthesia can only be upgraded by replacing the scanner unit with a Flex Focus 400 scanner unit. To get a complete Flex Focus system, you need to order both a scanner unit and a dock. 1202-7 (Flex Focus 200 Surgery) is an affordable surgical system with basic capabilities and limited surgical transducer support.

**1201-3**

1202-3 (Flex Focus 700) is a dedicated surgical system with touch screen. You need to order both a scanner unit and a dock.

## Power Pack

The Power Pack enables you to operate the system while it is not connected to an external electrical supply. It is located in the bottom drawer of the backpack. Only with Mobile Battery Keyboard Dock with battery UA1214 or Mobile Touch Dock with Battery UA1814.

**UA1247**

## Battery Charger Station

Like the Power Pack, but designed to stand on a table or hang on a wall.

## Docks

**UA1210**

### Mobile Keyboard Dock



**UA1211**

### Keyboard Wall Dock



**UA1214**

### Mobile Keyboard Dock

With battery

**UA1283**

### Keyboard Table Dock

**UA1810**

### Mobile Touch Dock

No DVD (RW) option

**UA1811**

### Touch Wall Dock

No DVD (RW) option

# Accessories for Flex Focus 1202

## Docks

**UA1814**

### Mobile Touch Dock
With battery

**UA1220**

### Backpack for Flex Focus
Transducer connector parking on top. Holds either two drawers, one drawer and a printer or the Battery Pack.

**UA1284-K**

### DVD Drive (upgrade)
Requires Keyboard Dock

**UA1237**



### Remote Control
For Flex Focus 700. Keys and mouse function to operate the system. Runs on two AA batteries.
Includes Mini Bluetooth Adapter.

**UA1285**

### Wheeled Transport Case
Suitcase on wheels for 1202. Holds:
- Scanner unit without dock
- Two transducers

**UA1294**

### Endo Transducer Holder
For mount on the array connector.

**UA1295**

### Endo Transducer Holder Mount
Dummy array connector for mechanical transducers without array connectors.

If you want to use Endo Transducer Holder UA1294 for 1850, 2050 or 2052, UA1295 is needed.

**UA1204**

### Wall-Mounted Transducer Holder Transducer Connector to mount on the wall (dummy)
Together with UA1204 this allows transducer storage on the wall, for instance near the sink.

# Accessories for Flex Focus 1202

**UA1308**

### Transducer Holder

For Flex Focus 1202

**UA1202**

### Foot Switch

For Pro Focus 2202 Ultraview and Flex Focus 1202

**AO0491**

### Video Cable (Flex Focus to phono and BNC)

Allows you to connect Flex Focus to video devices with phono and BNC sockets. 2.5 m long.

# 3D Imaging Accessories for Pro Focus 2202 and Flex Focus 1202

**UA0513**

### Magnetic Wheel Mover

Available for use with transducer types 8658, 8808, 8808e, 8818 and 8848 The mover is designed to rotate rectal ultrasound transducers in order to acquire a dataset that can be used to construct a 3D volume. It can be used as both a rotational mover and a pull-back mover.

**UA0510**

### Adapter Ring for 8848

For use with UA0513 as a rotational mover.

**UA0511**

### Adapter Ring for 8808

For use with UA0513 as a rotational mover.

**UA0512**

### Adapter Ring for 8818/8808e

For use with UA0513 as a rotational mover.

**UA0515**

### Pullback Adapter for 8848

For use with UA0513 as a pullback mover.

**UA0516**

### Pullback Adapter for 8818/8808e

For use with UA0513 as a pullback mover.

**EL4036**

### Adapter Cable for 1202

For use with UA0513 as a pullback mover.

**UA0553**

### Variable Friction Support Arm

Variable Friction Arm for UA0513 (Magnetic Wheel Mover)

**UA1215**

### Foot Switch

2-Pedal High-Quality Foot Switch. Both pedals are user-configurable when connected to 2202.

**UA1202**

### Foot Switch

For Pro Focus 2202 Ultraview and Flex Focus 1202

**UA0670**

### 3D Connector Box

Required for 3D connection to the following systems: 6503, 6503-2, 6503-4, 2202 with UA2202*.

*2202 is currently delivered with UA2223 which does not require a 3D Connector Box.

# Documentation Accessories

**EQ4042**

### Printing Paper SONY UPP-110HA

High density printing paper.
Roll size: 110 mm x 18 m.

For older printers.
Printer is no longer available.

**EQ4072**

### Printing Paper SONY UPP-110HG

High glossy printing paper.
Roll size: 110 mm x 20 m.
Print quantity: Approx. 217 prints per roll. 10 rolls of paper included with the printer.

**EQ4093**

### Color Printing Pack SONY UPC-21S

240 sheets of print paper.
3 rolls of ink ribbon.
Paper size: 100 x 90 mm.

**EQ4100**

### Digital B/W Printer SONY UP-D897

Digital Monochrome printer with a USB interface. The UP-D897 is a feature packed printer to allow for the greatest flexibility in black and white prints.
Part of Printer Start-Up Kit UA4100
Paper: EQ4072

**EQ4104**

### Digital B/W Printer SONY UP-D897 for Flex Focus 1202

Digital Monochrome printer with a USB interface. The UP-D897 is a feature packed printer to allow for the greatest flexibility in black and white prints.
Part of Printer Start-Up Kit UA4102
Paper: EQ4072

**EQ4105**

### Digital Color Printer SONY UP-D25MD for Pro Focus 2202 UltraView

Digital color dye sublimation printer with a USB interface. The UP-D25MD features a slim, compact design that is ideal for medical carts.
Paper: EQ4093 and EQ4094

**UA4102**

### Printer Start-Up Kit for Flex Focus 1202

Must be orderede separately. Consists of a SONY UP-D897 printer (EQ4104), a USB cable, a power cable and 10 rolls of printer paper.

# Power Cables

**AN0084**
2202 and 1202



**AN0089**
2202 and 1202

**AN0082**
2202 and 1202



**AN0081**
2202 and 1202

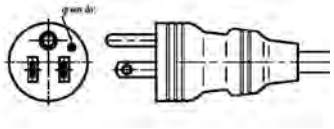

**AN0083**
2202 and 1202

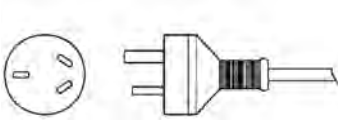

**AN0080**
2202 and 1202

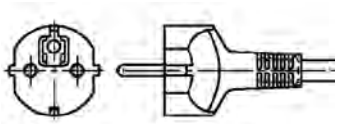

**AN0090**
2202 and 1202



(Reversed phase and null)

**AN0086**
2202 and 1202



Round pin

**AN0085**
2202 and 1202



**AN0087**
2202 and 1202



Flat pin

**AN0088**
2202 and 1202



# Power Cables

| COUNTRY | SIGNAL TYPE | COUNTRY CODE | 2202/1202 | VOLTAGE |
|---|---|---|---|---|
| ALBANIA | PAL B/G | 915 | AN0080 | 230 V |
| ALGERIA | PAL B/G | 903 | AN0080 | 230 V |
| ARGENTINA | PAL N | 921 | AN0090 | 230 V |
| AUSTRALIA | PAL B/G | 918 | AN0083 | 230 V |
| AUSTRIA | PAL B/G | 904 | AN0080 | 230 V |
| AZERBAIJAN | PAL B/G | 915 | AN0080 | 230 V |
| BAHRAIN | PAL B/G | 900 | AN0082 | 230 V |
| BANGLADESH | PAL B | 900 | AN0082 | 230 V |
| BELARUS | SECAM D/K | 915 | AN0080 | 230 V |
| BELGIUM (LUXEMBOURG) | PAL B/H | 901 | AN0080 | 230 V |
| BOLIVIA | NTSC M | 913 | AN0081 | 230 V |
| BOSNIA/HERZEGOVINA/ SERBIA | PAL B/H | 915 | AN0080 | 230 V |
| BRAZIL | PAL M | 914 | AN0081 | 115 V |
| BULGARIA | SECAM D/K | 992 | AN0080 | 230 V |
| CAMBODIA | "PAL B/G, NTSC M" | 900 | AN0082 | 230 V |
| CHILE | NTSC M | 923 | AN0085 | 230 V |
| CHINA (PEOPLE'S REPUB-LIC) | PAL D | 906 | AN0083 | 230 V |
| COLOMBIA | NTSC M | 913 | AN0081 | 115 V |
| COSTA RICA | NTSC M | 913 | AN0081 | 115 V |
| CROATIA | PAL B/H | 915 | AN0080 | 230 V |
| CUBA | NTSC M | 913 | AN0081 | 115 V |
| CYPRUS | PAL B/G | 983 | AN0082 | 230 V |
| CZECH REPUBLIC | "PAL B/G, SECAM D/K" | 982 | AN0080 | 230 V |
| DENMARK | PAL B/G | 974 | AN0087/AN0086 | 230 v |
| ECUADOR | NTSC M | 913 | AN0081 | 115 V |
| EGYPT | "PAL B/G, SECAM B/G" | 900 | AN0082 | 230 V |
| EL SALVADOR | NTSC M | 913 | AN0081 | 115 V |
| ESTONIA | "PAL B, SECAM D/K" | 984 | AN0080 | 230 V |
| FINLAND | PAL B/G | 908 | AN0080 | 230 V |
| FRANCE | SECAM L | 903 | AN0080 | 230 V |
| GEORGIA | SECAM D/K | 915 | AN0080 | 230 V |
| GERMANY | PAL B/G | 904 | AN0080 | 230 V |
| GHANA | PAL B/G | 900 | AN0082 | 230 V |
| GREECE | SECAM B/G | 910 | AN0080 | 230 V |
| GREENLAND | PAL B | 974 | AN0087/AN0086 | 230 V |
| GUATEMALA | NTSCM | 913 | AN0081 | 115 V |
| HONDURAS | NTSC M | 913 | AN0081 | 115 V |
| HONG KONG | PAL I | 924 | AN0082 | 230 V |
| HUNGARY | PAL K/K | 987 | AN0080 | 230 V |
| ICELAND | PAL B/G | 915 | AN0080 | 230 V |
| INDIA | PAL B | 917 | AN0084 | 230 V |
| INDONESIA | PAL B | 915 | AN0080 | 230 V |
| IRAN | SECAM B/G | 915 | AN0080 | 230 V |

# Power Cables

| COUNTRY | SIGNAL TYPE | COUNTRY CODE | 2202/1202 | VOLTAGE |
|---|---|---|---|---|
| IRAQ | SECAM B/G | 900 | AN0082 | 230 V |
| ISRAEL | PAL B/G | 919 | AN0089 | 230 V |
| ITALY | PAL B/G | 902 | AN0085 | 230 V |
| JAPAN | NTSC M | 905 | AN0081 | 115 V |
| JORDAN | PAL B/G | 900 | AN0082 | 230 V |
| KAZAKHSTAN | SECAM D/K | 915 | AN0080 | 230 V |
| KENYA | PAL B/G | 900 | AN0082 | 230 V |
| KUWAIT | PAL B/G | 900 | AN0082 | 230 V |
| LATVIA | "PAL B/G, SECAM D/K" | 985 | AN0080 | 230 V |
| LEBANON | PAL B/G | 900 | AN0082 | 230 V |
| LITHUANIA | "PAL B/G, SECAM D/K" | 986 | AN0080 | 230 V |
| MALAYSIA | PAL B | 900 | AN0082 | 230 V |
| MALTA | PAL B | 988 | AN0082 | 230 V |
| MEXICO | NTSC M | 913 | AN0081 | 115 V |
| MOROCCO | SECAM B | 903 | AN0080 | 230 V |
| NETHERLANDS | PAL B/G | 901 | AN0080 | 230 V |
| NEW ZEALAND | PAL B/G | 918 | AN0083 | 230 V |
| NIGERIA | PAL B/G | 900 | AN0082 | 230 V |
| NORWAY | PAL B/G | 976 | AN0080 | 230 V |
| OMAN | PAL B/G | 900 | AN0082 | 230 V |
| PAKISTAN | PAL B | 900 | AN0082 | 230 V |
| PERU | NTSC M | 907 | AN0080 | 230 V |
| PHILIPPINES | NTSC M | 916 | AN0081 | 230 V |
| POLAND | PAL B/G | 981 | AN0080 | 230 V |
| PORTUGAL | PAL B/G | 911 | AN0080 | 230 V |
| QATAR | PAL B | 900 | AN0082 | 230 V |
| ROMANIA | PAL D/G | 991 | AN0080 | 230 V |
| RUSSIA | SECAM D/K | 977 | AN0080 | 230 V |
| SAUDI ARABIA | "SECAM B/G, PAL B" | 900 | AN0082 | 230 V |
| SINGAPORE | PAL B/G | 900 | AN0082 | 230 V |
| SLOVAKIA | "PAL B, SECAM D/K" | 990 | AN0080 | 230 V |
| SLOVENIA | PAL B/H | 989 | AN0080 | 230 V |
| SOUTH AFRICA | PAL I | 917 | AN0084 | 230 V |
| SOUTH KOREA | NTSC M | 922 | AN0080 | 230 V |
| SPAIN | PAL B/G | 907 | AN0080 | 230 V |
| SWEDEN | PAL B/G | 975 | AN0080 | 230 V |
| SWITZERLAND | PAL B/G | 920 | AN0088 | 230 V |
| SYRIA | "SECAM B, PAL G" | 915 | AN0080 | 230 V |
| TAIWAN | NTSC | 905 | AN0081 | 115 V |
| THAILAND | PAL B/M | 916 | AN0081 | 230 V |
| TUNISIA | SECAM B/G | 903 | AN0080 | 230 V |
| TURKEY | PAL B | 915 | AN0080 | 230 V |
| UKRAINE | SECAM D/K | 915 | AN0080 | 230 V |
| URUGUAY | PAL N | 915 | AN0080 | 230 V |
| UNITED ARAB EMIRATES | PAL B/G | 900 | AN0082 | 230 V |

# Power Cables

| COUNTRY | SIGNAL TYPE | COUNTRY CODE | 2202/1202 | VOLTAGE |
|---|---|---|---|---|
| UNITED STATES (CANADA) | NTSC M | 909 | AN0081 | 115 V |
| UNITED KINGDOM | PAL I | 900 | AN0082 | 230 V |
| VENEZUELA | NTSC M | 913 | AN0081 | 115 V |
| VIETNAM | "NTSC M, SECAM D" | 915 | AN0080 | 230 V |
| YEMEN | PAL I | 915 | AN0082 | 230 V |

# Miscellaneous

**WQ0739**



### Scanning Gel

Electronic coupling medium for ultrasound imaging.
Refillable dispenser 290 ml.

Refill container 5 liters:
UA0610

**SC1474**

### OB Stickers for keyboard shortcuts

Extremely useful for users who use the programmable shortcuts in the obstetrics package to program shortcuts for advanced measurements. The stickers are placed on the shortcut keys you define.

**WQ0975**

### Breast Ultrasound Biopsy Phantom. Model 052

Training device for ultrasound guided biopsy procedures.
The phantom mimics the ultrasonic characteristics of tissues found in an average human breast.

**WQ0974**

### Tissue Equivalent Ultrasound Prostate Phantom. Model 053

Training device for imaging the prostate with a rectal transducer.

**WQ0970**

### Biplane Prostate Phantom

Training and simulation device. Organs and tissues are correctly adjusted to mimic exact Ultrasound echogenic seen by surgeon during OR procedures.

**WQ0971**

### Endfire Prostate Phantom

Training and simulation device. Organs and tissues are correctly adjusted to mimic exact Ultrasound echogenic seen by surgeon during OR procedures.

# Transducers and Transducer Accessories

## Endosonic Transducer 1850-M

*Systems: 2202 with Single Element Module UA2223/UA2223-K , 1202-1 and 1202-3*
*Frequency Range: 10-5 MHz* *Includes as standard: 1 transducer head, 1 tube and 1 hood. Must be specified when ordering. Type 1850-M without accessories: Order 1850-X or 1850-R (replacement)*




### Rectal Transducer — Type 6004

10 MHz, 90°

For transrectal examination.

WA0543

| | | |
|---|---|---|
| 17 mm Rectal Tube | UA0878 | Incl. lubricant and Rubber Sheaths UA0799. |
| Perenial Puncture Attachment | UA0650 | Bore diameter 2.1 mm. |
| Hood for UA0878 | WA0543 | |
| Hood for UA0878, plastic | EA4020 | Autoclavable. |

EA4020

| | | |
|---|---|---|
| Standoff Sheaths (box of 100) | UA0799 | Non-sterile for use with Rectal Tube UA0878. 1 box included with UA0878. |

UA0681

| | | |
|---|---|---|
| Inner Cylindrical Ring for UA0878 | YA0514 | |
| Outer Cylindrical Ring for UA0878 | YM1615 | |
| O-Rings for WA0543/EA4020 | YJ0621 | |
| Sterile, Single-Use Rectosigmoidoscope | UA0681 | With obturator and grip. |

UA0682

| | | |
|---|---|---|
| Light Source Cable Adapter for UA0681 | UA0682 | Reusable. For Storz and Wolf Light Sources. |




### Urethral and Rectal Transducer — Type 6005

10, 7.0 and 5.0 MHz, 90°

For transurethral and pediatric endoanal examination.

| | | |
|---|---|---|
| Tube for Type 6005. 10 mm | WA0500 | Incl. 2 hoods and Lubricant QS0011. |
| Extra hoods for WA0500, convex | WA0499 | |
| Extra hoods for WA0500, slim | WA0597 | |
| Extra hoods for WA0637 | WS3416 | |
| Storz Sheath | WQ0410 | |
| Adapter for WQ0410 | UA0652 | |

## Endosonic Transducer 1850-M (continued)




| | | |
|---|---|---|
| **Rectal Transducer**<br>10, 7.0 and 5.0 MHz, 90° | **Type 8539** | For transrectal examination.<br>Same accessories as for Type 6004. |
| Perineal Puncture Attachment | UA0650 | Bore diameter 2.1 mm. |
| Standoff Sheaths (box of 100) | UA0799 | Non-sterile for use with Rectal Tube UA0878. |
| Lubricant | QS0011 | |
| O-Ring for sealing between 1850-M and Rectal Tubes | YJ0632 | (proximal end of 1850-M) |
| O-Rings for crystals | YJ0619 | |
| Rasha Applicator | EA4006 | |
| Latex Covers | UA0069 | 24 pcs., Sterile, 3.2 cm tapered to 1.9 x 32 cm. |

# Transducers and Transducer Accessories

## Anorectal Transducers 2050 and 2052

*Systems: 2202 with Single Element Module UA2223/UA2223-K , 1202-1 and 1202-3*
*Frequency Range: 16-6 MHz*

UA0673

UA0681

UA0679

| | | |
|---|---|---|
| Carrying Case | KE4322 | Included. |
| **Water Standoff System:** | | |
| Water Standoff Collar | UA0671 | |
| Rectosigmoidoscope with obturator | UA0672 | For Welch Allyn® Light Source. |
| Rectosigmoidoscope with obturator | UA0673 | For Storz® Light Source. |
| Rectosigmoidoscope. Sterile, single-use* | UA0681 | With obturator and grip. |
| Non-Sterile Water Standoff Condoms, latex | UA0037 | 24 covers 2.6 x 30 cm. |
| Sterile Latex-Free Water Standoff Condoms | UA0068 | 24 pcs. |
| Light Source Cable Adapter for UA0681* | UA0682 | Reusable. For Storz and Wolf Light Sources. |
| Spare O-Rings for use with UA0671 | UA0674 | Pack of 10 Silicone O-Rings. |
| Glycerin-Based Lubricant | UA0675 | 250 ml for UA0037. |
| Plastic Extension Tube, 30 cm | UA0676 | (Included with UA0671 - can also be purchased separately). |
| 2-Way Stopcock | UA0677 | (Included with UA0671 - can also be purchased separately). |
| Plastic Syringe | UA0678 | (Included with UA0671 - can also be purchased separately). |
| CIDEX® Instrument Tray System | UA0061 | |
| **3D Imaging:** | | |
| 3D Connector Box | UA0670 | Required for 3D connection to the following systems: 6503, 6503-2, 6503-4, 2202 with UA2202**. |
| Variable Friction Support Arm | UA0553 | For use with Variable Friction Support Arm UA0553 |
| Transducer Support Collar | UA0679 | or any other clamp. |
| Sterile Latex Transducer Covers | UA0005 | 24 pcs. sterile transducer cover 2.6 x 20 cm. |

*Not released for sale in Canada

**2202 is delivered with UA2223 which does not require a 3D Connector Box.

# Transducers and Transducer Accessories

## Mechanical Sector Transducer 8551-R

*Systems: 2101 Premium with Single Element Module UA1255 or UA1255-K,*
*1101 with an integrated Single Element Module and 2202 Yellow, Green and Blue with Single Element Module,*
*Frequency Range: 10 - 6 MHz*
*Only sold as a replacement transducer*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Included. |
| Insert for Carrying Case | DS0524 | Included. |
| Extended Needle Guide for transrectal puncture | UC5299-E | 114.5 mm long. |
| Single-Use Cleaning Brush | QZ0040 | For needle guide. Included. |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| Latex Covers | UA0006 | 24 pcs., sterile covers 3.5 x 20 cm. |
| Latex Covers | UA0069 | 24 pcs., sterile, 3.2 cm tapered to 1.9 x 32 cm. |
| Water Stand-Off Rubber Sheath | UA0799 | 1 Pack of 100 included. Non-sterile. |
| Water Stand-Off O-Ring | QA0185 | 1 Pack of 100 included. Non-sterile. |

## Laparoscopic Transducer 8666-RF

*Systems: 2202 ,1202-3 and 1202-7*
*Frequency Range: 10-5 MHz*

UA1166

UA1249

| | | |
|---|---|---|
| Carrying Case | KE4320 | Included. |
| Biopsy Attachment | UA1249 | Needed for UA0039. |
| Histological Biopsy Needle Kit | UA0039 | 19 gauge needles needed. Box of 5 pcs. |
| No-Flex™ Attachment | UA1166 | For customers who prefer to image with a rigid laparoscopic transducer. |
| Single-Use Cleaning Brush, thin | QZ0040 | For needle guide. |
| NeoGuard® Sterile Covers | UA0067 | 12 pcs, telescopically folded, latex-free. |
| Leakage Testing Kit | UA1404 | |

# Transducers and Transducer Accessories

## Convex Array Transducer 8667

*Systems: 2202, 1202-1, 1202-2,1202-3 and 1202-7*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Needle Guide | UA1256 | Bore diameter of 1.5 mm and angle of insertion 0° to the long axis of the transducer. |
| Single-Use, Sterile Needle Guide | UA1256-U* | Bore diameter of 1.3 mm and angle of insertion 0° to the long axis of the transducer. 8 pcs. |
| Leakage Testing Kit | UA1404 | |
| Latex Covers | UA0006 | 24 pcs. sterile covers 3.5 x 20 cm. |
| CIV-Flex™ Latex-Free, Sterile Covers | UA0008 | 24 pcs11.97 cm narrowing down to 4.57 cm. |

* UA1256-U not released for sale in the USA and Canada

## Linear Array Transducer 8670

*Systems: 2202 and 1202*
*Frequency Range: 12-4 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |

UA1246

| | | |
|---|---|---|
| Needle Guide (for 8570 with 1101 and for 8670 with 1402 only) | UA1246 | Bore diameter 0.7-2.4 mm and angle of insertion of 45° to the image axis. Requires UA0028. |
| Needle Guide (For 8670 with 2202 and 1202 only) | UA1269 | Bore diameter 0.6-2.4 mm and angle of insertion of 30°, 45° and 60° to the image axis. |
| Needle Guide Insert for UA1246 | UA0028 | Box with 20 single-use inserts. |

UA1269

| | | |
|---|---|---|
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| CIV-Flex™ Sterile, Latex-Free Covers | UA0009 | 24 pcs. 8.89 x 60 cm. |
| CIV-Flex™ Sterile Covers, latex-free | UA0071 | 24 pcs., 8.9 x 91.5 cm, telescopically folded. |
| NeoGuard® Sterile Covers | UA0074 | 12 pcs., latex-free, 20.3 x 244 cm with SurgiTip 6 cm, telescopically folded. |

# Transducers and Transducer Accessories

## Convex Array Transducer 8802

*Systems: 2202, 1202-1 and 1202-3*
*Frequency Range: 6-3 MHz*

| | | | |
|---|---|---|---|
| | Carrying Case | KE4300 | Must be ordered separately. |
| UA1250 | Needle Guide | UA1250 | Bore diameter variable from 0.6 to 2.4 mm and angle of insertion 18° to the long axis of the transducer. |
| | Leakage Testing Kit | UA1404 | |
| | Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| | CIV-Flex™ Sterile, Latex-Free Covers | UA0009 | 24 pcs. 8.89 x 60 cm. |
| | CIV-Flex™ Sterile Covers, latex-free | UA0071 | 24 pcs., 8.9 x 91.5 cm, telescopically folded. |
| | CIV-Flex™ Cover, latex-free | UA0076 | 24 pcs., 14 x 147 cm, telescopically folded. |

# Transducers and Transducer Accessories

## Biplane Transducer 8808

*Systems: 2202, 1202-1, 1202-2, 1202-3 and 1202-7*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Dummy Channel Bracket | UA1272 | Included. |

### Transrectal Biopsy Guides

| | | |
|---|---|---|
| Reusable Biopsy Guide | UA1257-R17 | For 17-gauge needles. Includes: |
| | UA1257 | Biopsy Channel Bracket |
| | UC5296 | 17-gauge needle guide |
| Extended, Reusable Biopsy Guides | UA1257R17E | For 17-gauge needles. Long needle guide. Includes: |
| | UA1257 | Biopsy Channel Bracket |
| | UC5296-E | 17-gauge long needle guide |

UA1257-S14

| | | |
|---|---|---|
| Reusable Biopsy Guide | UA1257-R14 | For 14-gauge needles. Includes: |
| | UA1257 | Biopsy Channel Bracket |
| | UC5298 | 14-gauge needle guide |

UA1257S17E

| | | |
|---|---|---|
| Single-Use Biopsy Guides | UA1257-S14 | For 14-gauge needles. Sterile packed. 18 pcs. |
| Extended, Single-Use Biopsy Guides | UA1257S17E | For 17-gauge needles. Sterile-packed. 18 pcs. Includes: Biopsy Channel Bracket 17-gauge needle guide |

UA1232

| | | |
|---|---|---|
| Transperineal Puncture Attachment | UA1232 | Bore diameter of 2.2 mm and angle of insertion 0° to the long axis of the transducer. |

| | | |
|---|---|---|
| Single-Use Cleaning Brush, thin | QZ0040 | For needle guide. |
| Magnetic Wheel Mover for 3D Imaging | UA0513 | |
| Mover Adapter Ring for UA0513 | UA0511 | |
| Variable Friction Support Arm | UA0553 | For Magnetic Wheel Mover. |
| Rubber Water Standoff Sheaths | UA0799 | Non-sterile. Pack of 100. |
| Water Standoff O-Rings | UA0210 | Non-sterile. Pack of 100. |
| Leakage Testing Kit | UA1404 | |
| CIV-Flex™ Latex-Free, Sterile Covers | UA0008 | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |
| Latex Covers | UA0032 | 24 pcs., non-sterile. |
| Latex Covers | UA0069 | 24 pcs., sterile, 3.2 cm tapered to 1.9 x 32 cm. |

# Transducers and Transducer Accessories

## Endorectal Biplane Transducer 8808e

*Systems: 2202 , 1202-1, 1202-2, 1202-3 and 1202-7*
*Frequency Range: 10-5 MHz*

UA 1324

| | | |
|---|---|---|
| Dummy Channel Bracket | UA1325 | Included. |
| Carrying Case | KE4300 | Must be ordered separately. |
| Simultaneous Biplane Biopsy Guides | UA1326 | Reusable. Bore diameter 1.6 mm; angle of insertion 19° to the long axis of the transducer. |
| Single-Use Biplane Biopsy Guides | UA1322-S | Sterile packed. 18 pcs. Bore diameter of 1.6 mm; angle of insertion 19° to the long axis of the transducer. |
| Single-Use Biplane Biopsy Guides | UA1322-S14 | Sterile packed. 18 pcs. Bore diameter of 2.1 mm; angle of insertion 19° to the long axis of the transducer. |
| Single-Use Cleaning Brush, thin | QZ0040 | For needle guide. |
| Perineal Puncture Attachment | UA1324 | Bore diameter 2.1 mm; angle of insertion 0° to the long axis of the transducer. |
| Civco Multi-Purpose Workstation | UA2020 | For transperineal biopsies. |
| Magnetic Wheel Mover for 3D Imaging | UA0513 | |
| Mover Adapter Ring for UA0513 | UA0512 | |
| Variable Friction Support Arm | UA0553 | For Magnetic Wheel Mover. |
| Pullback Adapter | UA0516 | For Magnetic Wheel Mover. |
| Leakage Testing Kit | UA1404 | |
| CIV-Flex™ Latex-Free, Sterile Covers | UA0008 | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |
| Latex Covers | UA0032 | 24 pcs., non-sterile. |
| Latex Covers | UA0069 | 24 pcs., sterile, 3.2 cm tapered to 1.9 x 32 cm. |

# Transducers and Transducer Accessories

## Linear Array Transducer 8809

*Systems: 2202 , 1202-1, 1202-3 and 1202-4*
*Frequency Range: 15-6 MHz*

UA1262

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Transducer Holder | DZ9756 | Included. |
| Needle Guide | UA1262 | Can be used with needles up to 1.2 mm/18 gauge. |
| Leakage Testing Kit | UA1404 | |
| Sterile Cable Covers, latex-free | UA0004* | 24 pcs. 2.5 m. |
| CIV-Flex™ Latex-Free, Sterile Covers | UA0008* | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |
| NeoGuard® Covers, latex-free | UA0075 | 12 pcs., 15.2 x 244 cm plus form-fitted NeoGuard® tip, telescopically folded. |

* Must be used together

## Linear Array Transducer 8811

*Systems: 2202 and 1202*
*Frequency Range: 12-5 MHz*

UA1239

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Needle Guide | UA1239 | Bore diameter up to 2.1 mm and angle of insertion 30°, 45° and 60° to the image axis. |
| Leakage Testing Kit | UA1404 | |
| CIV-Flex™ Covers | UA0007 | 24 pcs. sterile covers 13.97 x 60 cm. |
| CIV-Flex™ Sterile Covers, latex-free | UA0070 | 24 pcs., 14 x 91 cm, telescopically folded. |
| NeoGuard® Sterile Covers | UA0074 | 12 pcs., latex-free, 20.3 x 244 cm with SurgiTip 6 cm, telescopically folded. |

# Transducers and Transducer Accessories

## Linear Array Transducer 8812

*Systems: 2202*
*Frequency Range: 8-3.75 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |

UA1246

| | | |
|---|---|---|
| Needle Guide | UA1246 | Bore diameter of 0.7-2.7 mm and angle of insertion 0f 45° to the image axis. Requires UA0028. |
| Single-Use Needle Cartridges | UA0028 | Box of 20. Single-use. |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| CIV-Flex™ sterile, Latex-Free Covers | UA0009 | 24 pcs. 8.89 x 60 cm. |
| CIV-Flex™ sterile Covers, latex-free | UA0071 | 24 pcs., 8.9 x 91.5 cm, telescopically folded. |
| NeoGuard® Sterile Covers | UA0074 | 12 pcs., latex-free, 20.3 x 244 cm with SurgiTip 6 cm, telescopically folded. |

## Intraoperative Transducer 8814

*Systems: 2202, 1202-3*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Transducer Holder | DZ9756 | Included. |
| Instructions for use | BB1943 | Included. |
| Carrying Case | KE4300 | Must be ordered separately. |

UA1335

| | | |
|---|---|---|
| Single-Use Needle Guide | UA1335 | Box of 9. |
| Leakage Testing Kit | UA1404 | |
| Sterile cable Covers, latex-free | UA0004* | 24 pcs. 2.5 m. Used with UA0009. |
| CIV-Flex™ Sterile, Latex-Free Covers | UA0009* | 24 pcs. 8.89 x 60 cm. Used with UA0004. |
| NeoGuard® Sterile Covers | UA0074 | 12 pcs., latex-free, 20.3 x 244 cm with SurgiTip. 6 cm, telescopically folded. |

*Must be used together

# Transducers and Transducer Accessories

## Intraoperative Transducer 8815

*Systems: 2202, 1202-3 and 1202-7*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Transducer Holder | DZ9756 | Included. |
| Carrying Case | KE4300 | Must be ordered separately. |
| Single-Use Needle Guide | UA1336 | Includes: 3-angle insert for 10-20 gauge needles (box of 9), Free-angle insert for 10-20 gauge needles (box of 9). |
| Leakage Testing Kit for 8815 | UA1404 | |
| Sterile Cable Covers, latex-free | UA0004* | 24 pcs. 2.5 m. |
| CIV-Flex™ Latex-Free, sterile covers | UA0008* | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |
| Sterile Latex Transducer Covers | UA0005 | 24 pcs. sterile transducer cover 2.6 x 20 cm. |
| NeoGuard® SurgiTip Covers, sterile | UA0073 | 12 pcs., latex-free, 15.2 x 244 cm with SurgiTip. 3 cm, telescopically folded (recommended). |

UA1336

* Must be used together

## T-Shaped Intraoperative Transducer 8816

*Systems: 2202, 1202-3, 1202-4 and 1202-7*
*Frequency Range: 10-4 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | |
| Insert for Carrying Case | DS0976 | |
| Transducer Holder | DZ9756 | |
| Leakage Testing Kit | UA1404 | |
| Sterile Cable Covers, latex-free | UA0004* | 24 pcs. 2.5 m. |
| CIV-Flex™ Sterile, Latex-Free Covers | UA0009* | 24 pcs. 8.89 x 60 cm. |
| NeoGuard® SurgiTip Covers, sterile | UA0073 | 12 pcs., latex-free, 15.2 x 244 cm with SurgiTip. 3 cm, telescopically folded (recommended). |

* Must be used together

# Transducers and Transducer Accessories

## Biplane and Endfire Transducer 8818

*Systems: 2202, 1202-1 and 1202-3*
*Frequency Range: 12-4 MHz*

UA1329-S

UA1324

| | | |
|---|---|---|
| Dummy Channel Bracket | UA1325 | Included. |
| Carrying Case | KE4300 | Must be ordered separately. |
| Civco Multi-Purpose Workstation | UA2020 | For transperineal biopsies. |
| Endfire Biopsy Guides* | UA1327 | Reusable. Bore diameter 1.6 mm; angle of insertion 0° to the long axis of the transducer. |
| | UA1323-S | Single-use, sterile packed. 18 pcs. |
| Simultaneous Biplane Biopsy Guides* | UA1326 | Reusable. Bore diameter 1.6 mm; angle of insertion 19° to the long axis of the transducer. |
| | UA1322-S | Single-use, sterile packed. 18 pcs. |
| | UA1322-S14 | Sterile packed. 18 pcs. Bore diameter of 2.1 mm; angle of insertion 19° to the long axis of the transducer. |
| Dual Biopsy Guides* | UA1328 | Reusable. Bore diameter 1.6 mm; angle of insertion 0° and 19° to the long axis of the transducer. |
| | UA1329-S | Single-use, sterile packed. 18 pcs. |
| Perineal Puncture Guide | UA1324 | Perineal puncture attachment. Bore diameter 2.1 mm; angle of insertion 0° to the long axis of the transducer. |
| Single-Use Cleaning Brush, thin | QZ0040 | For needle guide. |
| Leakage Testing Kit | UA1404 | |
| Magnetic Wheel Mover for 3D Imaging | UA0513 | |
| Mover Adapter Ring | UA0512 | |
| Variable Friction Support Arm | UA0553 | For Magnetic Wheel Mover. |
| Pullback Adapter | UA0516 | For Magnetic Wheel Mover. |
| CIV-Flex™ Latex-Free, sterile covers | UA0008 | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |
| Latex Covers | UA0032 | 24 pcs., non-sterile. |
| Latex Covers | UA0069 | 24 pcs., sterile, 3.2 cm tapered to 1.9 x 32 cm. |

* All biopsy guides include needle guides

# Transducers and Transducer Accessories

## Endovaginal Endfire Transducer 8819

*Systems: 2202, 1202-1,1202-2, 1202-3 and 1207-7*
*Frequency Range: 9-6 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4325 | |
| Insert for Carrying Case | DS0537 | |
| Needle Guide | UA1282 | Bore diameter 1.8 mm; angle of insertion 0.9° to the long axis of the transducer. Includes 3 single-use cleaning brushes. |
| Single-Use Cleaning Brush, thin | QZ0040 | For needle guide. |
| CIVCO Sterile Endocavity Needle Guide | 610-958 | To purchase, please contact your CIVCO supplier. |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| Sterile Latex Transducer Covers | UA0005 | 24 pcs. sterile covers 2.6 x 30 cm. |
| CIV-Flex™ Latex-Free, Sterile Covers | UA0008 | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |

UA1282

## Convex Array Transducer 8820e

*Systems: 2202, 1202-1, 1202-2 , 1202-3 and 1202-7*
*Frequency Range: 6-2 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Needle Guide | UA1250 | Bore diameter variable from 0.6 to 2.4 mm and angle of insertion 18° to the long axis of the transducer. |
| Needle Guide Kit | UA1341 | Including: 1 reusable bracket, 5 sterile Ultra-Pro 3™ needle guides with transducer cover and gel. |
| Sterile Ultra-Pro 3™ Needle Guides | UA0013 | 24 pcs. |
| Leakage Testing Kit | UA1404 | |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| CIV-Flex™ Sterile, Latex-Free Covers | UA0009 | 24 pcs. 8.89 x 60 cm. |
| CIV-Flex™ Covers | UA0007 | 24 pcs. sterile covers 13.97 x 60 cm. |
| CIV-Flex™ Sterile Covers, latex-free | UA0070 | 24 pcs., 14 x 91 cm, telescopically folded |
| Sterile Latex Covers, intraoperative | UA0072 | 12 pcs., 20.3 x 244 cm with 9 cm tip, telescopically folded. |
| CIV-Flex™ Covers, latex-free | UA0076 | 24 pcs., 14 x 147 cm, telescopically folded. |

UA1341 with UA0013

# Transducers and Transducer Accessories

## Vascular Transducer 8822

*Systems: 2202, 1202-1 and 1202-3*
*Frequency Range: 9-3.5 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Needle Guide | UA1239 | Bore diameter up to 2.1 mm and angle of insertion 30°, 45° and 60° to the image axis. |
| Leakage Testing Kit | UA1404 | |

UA1239

| | | |
|---|---|---|
| CIV-Flex™ Covers | UA0007 | 24 pcs. sterile covers 13.97 x 60 cm. |
| CIV-Flex™ Sterile Covers, latex-free | UA0070 | 24 pcs., 14 x 91 cm, telescopically folded. |
| NeoGuard® Sterile Covers | UA0074 | 12 pcs., latex-free, 20.3 x 244 cm with SurgiTip 6 cm, telescopically folded. |

## Convex Array Transducer 8823

*Systems: 2202 and 1202*
*Frequency Range: 6-1.8 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |

UA1250

| | | |
|---|---|---|
| Needle Guide | UA1250 | Bore diameter variable from 0.6 to 2.4 mm and angle of insertion 18° to the long axis of the transducer. |
| Needle Guide Kit | UA1341 | Including: 1 reusable bracket, 5 sterile Ultra-Pro 3™ needle guides with transducer cover and gel. |
| Sterile Ultra-Pro 3™ Needle Guides | UA0013 | 24 pcs. |
| Leakage Testing Kit | UA1404 | |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| CIV-Flex™ sterile, Latex-Free Covers | UA0009 | 24 pcs. 8.89 x 60 cm. |
| CIV-Flex™ Sterile Covers, latex-free | UA0071 | 24 pcs., 8.9 x 91.5 cm, telescopically folded. |
| CIV-Flex™ Cover, latex-free | UA0076 | 24 pcs., 14 x 147 cm, telescopically folded. |

UA1341 with UA0013

# Transducers and Transducer Accessories

## I and T Shaped Intraoperative Transducer 8824

*Systems: 2202 and 1202-3*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Carrying Case | KP0212 | Must be ordered separately. |
| Insert for Carrying Case | DS0977 | |
| Single-Use Needle Guide Kit | UA1337 | Box of 9. |
| UA1337 includes: | | 2 needle guide insert palettes (3-angle and free-angle respectively), each with 9 different inserts for 10-20 gauge needles. |
| Leakage Testing Kit | UA1404 | |
| Sterile Cable Covers, latex-free | UA0004* | 24 pcs. 2.5 m. |
| CIV-Flex™ Latex-Free, sterile covers | UA0008* | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |
| NeoGuard® SurgiTip Covers, sterile | UA0073 | 12 pcs., latex-free, 15.2 x 244 cm with SurgiTip 3 cm, telescopically folded (recommended). |

UA1337

* Must be used together

## ProART Robotic Transducer 8826

*Systems: 2202-7 and 1202-3*
*Frequency Range: 12-4.3 MHz (depending on system)*

| | | |
|---|---|---|
| Carrying Case | KE4320 | Included. |
| Leakage Testing Kit | UA1404 | |
| Latex-Free Laparoscopic Transducer Cover | UA0067 | 12 pcs. Telescopically folded (not suitable for robotic surgery). |

# Transducers and Transducer Accessories

## Convex Array Transducer 8830

*Systems: 1202*
*Frequency Range: 6-2 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |

UA1250

| | | |
|---|---|---|
| Needle Guide | UA1250 | Bore diameter variable from 0.6 to 2.4 mm and angle of insertion 18° to the long axis of the transducer. |
| Needle Guide Kit | UA1341 | Including: 1 reusable bracket, 5 sterile Ultra-Pro 3™ needle guides with transducer cover and gel. |
| Sterile Ultra-Pro 3™ Needle Guides | UA0013 | 24 pcs. |

UA1341 with UA0013

| | | |
|---|---|---|
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs., 2.5 m. |
| CIV-Flex™ Sterile Covers | UA0007 | 24 pcs., 2.5 m. |
| CIV-Flex™ Sterile, Latex-Free Covers | UA0009 | 24 pcs., 13.97 x 60 cm. |
| CIV-Flex™ Sterile Covers, latex-free | UA0070 | 24 pcs., 8.89 x 60 cm. |
| Sterile Latex Covers, intraoperative | UA0072 | 24 pcs., 14 x 91 cm, telescopically folded.<br>12 pcs., 20.3 x 244 cm with 9 cm tip, telescopically folded. |
| CIV-Flex™ Covers, latex-free | UA0076 | 24 pcs., 14 x 147 cm, telescopically folded. |

# Transducers and Transducer Accessories

## 3D*ART* Transducer 8838

*Systems: 2202 with 3D Professional UA2222 and Single Element Module UA2223, 1202-1 and 1202-3 with 3D Professional UA1222*

*Frequency Range: 12-4 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4325 | Included. |
| Insert for Carrying Case | DS0980 | Included. |
| Endo Transducer Holder Insert for Pro Focus 2202 UltraView | UA1347 | |
| Transducer Holder for Flex Focus 1202 | UA1308 | |
| Robotic Stationary Transducer (RST)™ Arm | UD1309 | Designed to hold the transducer during robotic-assisted surgery procedures. |
| General Transducer Holder | UA1296 | For Flex Focus 1202 Mobile Touch Docks UA1810 and UA1814. |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs., 2.5 m. |
| Sterile Latex Transducer Covers | UA0006 | 24 pcs. sterile covers 3.5 x 20 cm. |
| Sterile Latex Transducer Covers | UA0069 | 24 pcs., sterile, 3.2 cm tapered to 1.9 x 32 cm. |

# Transducers and Transducer Accessories

## Transducer 8848

*Systems: 2202, 1202-1 and 1202-3*
*Frequency Range: 12-4 MHz*

UA1232

| | | |
|---|---|---|
| Carrying Case | KE4326 | Must be ordered separately. |
| Needle Guide | UA1232 | Bore diameter variable of 2.2 mm and angle of insertion 0° to the long axis of the transducer. |
| CIV Flex Brachy Balloons, latex-free | UA0059 | 10 pcs. |
| CIVCO Classic Stepper and Micro-Touch® Stand | UA2000 | See page 39 for more details. |
| CIVCO Classic Stepper and Micro-Touch® Stand | UA2001 | See page 39 for more details. |
| EXII Tracked Stepper and Stand | UA2010 | See page 39 for more details. |
| EXII Tracked Stepper and Stand | UA2011 | See page 39 for more details. |
| Magnetic Wheel Mover for 3D Imaging | UA0513 | |
| Mover Adapter Ring | UA0510 | |
| Variable Friction Support Arm | UA0553 | For Magnetic Wheel Mover. |
| Pullback Adapter | UA0515 | For Magnetic Wheel Mover. |
| Sterile Latex Transducer Covers | UA0005 | 24 pcs. sterile transducer cover 2.6 x 20 cm. |
| CIV-Flex™ Latex-Free, sterile covers | UA0008 | 24 pcs. 11.97 cm narrowing down to 4.57 cm. |

## Craniotomy Transducer 8862

*Systems: 2202, 1202-1 and 1202-3*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Transducer Holder | DZ9756 | Included. |
| Assembly Guide for UA1345 | BB2080 | |
| Needle Guide | UA1345 | Single-Use, Sterile Packed, Needle Guide Kit (box of 9). Includes 1 needle guide and 2 needle guide insert palettes (3-angle and free-angle respectively), each with 9 different inserts for 10-20 gauge needles. |
| NeoGuard® SurgiTip Covers, sterile | UA0073 | 12 pcs., latex-free, 15.2 x 244 cm with SurgiTip 3 cm, telescopically folded (recommended). |

# Transducers and Transducer Accessories

## Burr Hole Transducer 8863

*Systems: 1202-3 and 2202-7*
*Frequency Range: 10-5 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |
| Transducer Holder | DZ9756 | Included. |
| Assembly guide for UA1346* | BB2080 | |
| Needle Guide | UA1346 | Single-Use, Sterile Packed, Needle Guide Kit (box of 9). Includes 1 palette with needle guide and 9 different inserts for 10-20 gauge needles. |
| Leakage Testing Kit | UA1404 | |
| NeoGuard® SurgiTip Covers, sterile | UA0073 | 12 pcs., latex-free, 15.2 x 244 cm with SurgiTip 3 cm, telescopically folded (recommended). |

*For future release

## High Frequency Linear Array Transducer 8870

*Systems: 2202-7, 1202-1, 1202-3 and 1202-4*
*Frequency Range: 18-6 MHz*

| | | |
|---|---|---|
| Carrying Case | KE4300 | Must be ordered separately. |

UA1251

| | | |
|---|---|---|
| Needle Guide | UA1251 | Bore diameter variable from 0.6-3.4 mm; angle of insertion of 30, 45 or 60° to the long axis of the transducer. |
| Sterile Cable Covers, latex-free | UA0004 | 24 pcs. 2.5 m. |
| CIV-Flex™ Sterile, Latex-Free Covers | UA0009 | 24 pcs. covers 13.97 x 60 cm. |

## CIVCO AccuCare Stepper Units (Barzell-Whitmore)

CIVCO AccuCare Micro-Touch® Stepper

For transducer:
8848

| | | |
|---|---|---|
| CIVCO Classic Stepper and Micro-Touch® stand. Table mount. | UA2000 | Including 2 x 5 18G Templates (UA2005), 20 Sterile Drapes (UA2007) and 10 Non-Sterile Brachy Balloons (UA0059). |
| CIVCO Classic Stepper and Micro-Touch® stand. Table mount. | UA2001 | Including 2 x 5 17G Templates (UA2006), 20 Sterile Drapes (UA2007) and 10 Non-Sterile Brachy Balloons (UA0059). |
| EXII Tracked Stepper and Micro-Touch® stand. Table mount. | UA2010 | Including 2 x 5 18G Templates (UA2005), 20 Sterile Drapes (UA2007) and 10 Non-Sterile Brachy Balloons (UA0059). |
| EXII Tracked Stepper and Micro-Touch® stand. Table mount. | UA2011 | Including 2 x 5 17G Templates (UA2006), 20 Sterile Drapes (UA2007) and 10 Non-Sterile Brachy Balloons (UA0059). |
| CIVCO Multi-Purpose Workstation | UA2020 | |

**Options:**

| | | |
|---|---|---|
| CIV Flex Brachy Balloons, latex-free | UA0059 | 10 pcs. |
| Sterile, Single-Use 18G Templates | UA2005 | 1 box = 5 units. Min. order 2 boxes. |
| Sterile, Single-Use 17G Templates | UA2006 | 1 box = 5 units. Min. order 2 boxes. |
| Sterile Drapes | UA2007 | 1 box = 20 units. |

# Index of Reference Numbers


## Systems

1202 ***1***
1202-1 ***1***
1202-2 ***1***
1202-3 ***1***
1202-4 ***1***
1202-7 ***1***
2202 ***1***
2202- 7 ***1***
2202-2 ***1***
2202-7 ***2***
2202-9 ***1***
610-958 ***31***

## A

AN0080 ***14***
AN0081 ***14***
AN0082 ***14***
AN0083 ***14***
AN0084 ***14***
AN0085 ***14***
AN0086 ***14***
AN0087 ***14***
AN0088 ***14***
AN0089 ***14***
AN0090 ***14***
AO0421 ***7***
AO0491 ***5***, ***11***

## B

BB1943 ***28***
BB2080 ***36***, ***37***

## D

DP0925 ***7***
DS 0977 ***33***
DS0524 ***22***
DS0537 ***31***
DS0967 ***7***
DS0976 ***29***
DS0977 ***33***
DS0980 ***35***
DZ 9756 ***36***
DZ9756 ***7***, ***27***, ***28***, ***29***, ***36***, ***37***
DZ9772 ***8***

## E

EA4006 ***20***
EA4020 ***19***
EL4036 ***12***
EQ4042 ***13***
EQ4072 ***13***
EQ4093 ***13***
EQ4100 ***13***
EQ4102 ***8***
EQ4104 ***13***
EQ4105 ***13***

## K

KE1325 ***26***, ***30***
KE4300 ***22***, ***23***, ***24***, ***25***, ***26***, ***27***, ***28***, ***29***, ***30***, ***31***, ***32***, ***34***, ***36***, ***37***
KE4320 ***22***, ***33***
KE4322 ***21***
KE4325 ***31***, ***35***
KE4326 ***36***
KP0212 ***33***

## N

NP0959 ***8***

## Q

QA0185 ***22***
QA0228 ***5***, ***7***
QS0011 ***20***
QZ 0040 ***26***
QZ0040 ***22***, ***25***, ***30***, ***31***

## S

SC1474 ***18***
SC1624 ***8***

## U

UA0004 ***22***, ***23***, ***24***, ***27***, ***28***, ***29***, ***31***, ***32***, ***33***, ***34***, ***35***, ***36***, ***37***
UA0005 ***21***, ***29***, ***31***, ***36***, ***37***
UA0006 ***22***, ***23***, ***35***
UA0007 ***27***, ***31***, ***32***, ***34***
UA0008 ***23***, ***25***, ***26***, ***27***, ***29***, ***30***, ***31***, ***33***, ***36***
UA0009 ***23***, ***24***, ***28***, ***29***, ***31***, ***32***, ***34***, ***37***
UA0013 ***31***, ***32***, ***34***
UA0028 ***23***, ***28***
UA0032 ***25***, ***26***, ***30***
UA0037 ***21***
UA0039 ***22***
UA0040 ***22***
UA0058 ***38***
UA0059 ***36***, ***38***
UA0061 ***21***
UA0067 ***22***, ***33***
UA0069 ***20***, ***22***, ***25***, ***26***, ***30***, ***35***
UA0070 ***27***, ***31***, ***32***, ***34***
UA0071 ***23***, ***24***, ***28***, ***32***
UA0072 ***31***, ***34***
UA0073 ***29***, ***33***, ***36***, ***37***
UA0074 ***23***, ***27***, ***28***, ***32***
UA0075 ***27***
UA0076 ***7***, ***24***, ***31***, ***32***, ***34***
UA0210 ***25***
UA0510 ***12***, ***36***
UA0511 ***12***, ***25***
UA0512 ***12***, ***26***, ***30***

# Index of Reference Numbers


UA0513 ***12***, ***25***, ***26***, ***30***, ***36***
UA0515 ***12***, ***36***
UA0516 ***12***, ***26***, ***30***
UA0553 ***12***, ***21***, ***25***, ***26***, ***30***, ***36***
UA0610 ***18***
UA0650 ***19***, ***20***
UA0652 ***19***
UA0670 ***12***, ***21***
UA0671 ***21***
UA0672 ***21***
UA0673 ***21***
UA0674 ***21***
UA0675 ***21***
UA0676 ***21***
UA0677 ***21***
UA0678 ***21***
UA0679 ***21***
UA0681 ***19***, ***21***
UA0682 ***19***, ***21***
UA0799 ***19***, ***20***, ***22***, ***25***
UA0878 ***19***
UA0955 ***8***
UA0964 ***5***
UA1166 ***22***
UA1202 ***5***, ***7***, ***11***, ***12***
UA1203 ***4***
UA1204 ***4***, ***10***
UA1206 ***4***
UA1207 ***4***
UA1210 ***4***, ***9***
UA1211 ***4***, ***9***
UA1214 ***9***
UA1215 ***7***, ***12***
UA1220 ***5***, ***10***
UA1222 ***4***
UA1223 ***5***
UA1225 ***5***
UA1226 ***4***
UA1232 ***25***, ***36***
UA1237 ***4***, ***10***
UA1239 ***27***, ***32***
UA1246 ***23***, ***28***
UA1247 ***5***, ***9***
UA1249 ***22***
UA1250 ***24***, ***31***, ***32***, ***34***
UA1251 ***37***
UA1256 ***23***
UA1256-U ***23***
UA1257 ***25***
UA1257-R14 ***25***
UA1257-R17 ***25***
UA1257R17E ***25***
UA1257-S14 ***25***
UA1257S17E ***25***
UA1258 ***4***
UA1262 ***27***
UA1269 ***23***
UA1271 ***7***
UA1272 ***25***
UA1282 ***31***
UA1283 ***4***, ***9***
UA1284 ***10***
UA1284-K ***5***
UA1285 ***5***, ***10***
UA1294 ***4***, ***10***
UA1295 ***4***, ***10***, ***11***
UA1296 ***5***, ***35***
UA1298 ***4***
UA1302 ***8***
UA1308 ***35***
UA1322-S ***26***, ***30***
UA1322-S14 ***26***, ***30***
UA1323-S ***30***
UA1324 ***26***, ***30***
UA1326 ***26***, ***30***
UA1327 ***30***
UA1328 ***30***
UA1329-S ***30***
UA1329-S1 ***30***
UA1335 ***28***
UA1336 ***29***
UA1337 ***33***
UA1341 ***31***, ***32***, ***34***
UA1345 ***36***
UA1346 ***37***
UA1347 ***35***
UA1404 ***22***, ***23***, ***24***, ***25***, ***26***, ***27***, ***28***, ***29***, ***30***, ***31***, ***32***, ***33***, ***37***
UA1414 ***33***
UA1810 ***4***, ***9***
UA1811 ***4***, ***9***
UA1814 ***4***, ***10***
UA2000 ***36***, ***38***
UA2001 ***36***, ***38***
UA2005 ***38***
UA2006 ***38***
UA2007 ***38***
UA2010 ***36***, ***38***
UA2011 ***36***, ***38***
UA2020 ***26***, ***30***, ***38***
UA2204 ***7***
UA2205 ***2***, ***4***
UA2206 ***2***
UA2207 ***2***
UA2214 ***2***
UA2215 ***2***
UA2220 ***2***
UA2222 ***2***
UA2222-K ***2***
UA2223 ***2***
UA2223-K ***2***
UA2226 ***2***
UA2226-K ***2***
UA2229-K ***3***
UA2233-K ***3***
UA2235 ***2***
UA2235-K ***2***

# Index of Reference Numbers


UA2236 ***2***
UA2236-K ***2***
UA2237-K ***2***
UA2238 ***2***
UA2238-K ***2***
UA2240 ***8***
UA2251 ***2***
UA2251-K ***2***
UA2252 ***2***
UA2252-K ***2***
UA2410 ***3***, ***7***
UA4100 ***3***, ***8***
UA4102 ***5***, ***13***
UC5296 ***25***
UC5296-E ***25***
UC5298 ***25***
UC5299-E ***22***
UD1309 ***35***

**W**
WA0499 ***19***
WA0500 ***19***
WA0543 ***19***
WA0597 ***19***
WQ0410 ***19***
WQ0739 ***18***
WQ0970 ***18***
WQ0971 ***18***
WQ0974 ***18***
WQ0975 ***18***
WS3416 ***19***

**Y**
YA0514 ***19***
YJ0619 ***20***
YJ0621 ***19***
YJ0632 ***20***
YM1615 ***19***

# To order, Please contact

MANUFACTURER
BK Medical ApS
Mileparken 34
DK-2730 Herlev
Denmark

Headquarters USA:
B-K Medical Systems, Inc.
8 Centennial Drive
Peabody, MA 001960
USA
Tel.: (1) 978-326-1300
Fax: (1) 978-326-1399

B-K Medical Benelux
Generaal de Wittelaan 19/7
2800 Mechelen
Belgium
Tel.: (32) 1528 0600
Fax: (32) 1529 1025

B-K Medical Medizinische systeme GmbH
Pascalkehre 13
25451 Quickborn
Germany
Tel: (49) 4106 99 55-0
Fax: (49) 4106 99 55-99

B-K Medicale S.r.l.
Via Tulipani, 3/B
20090 Pieve Emanuele MI
Italy
Tel.: (39) 02 90 78 13 47
Fax: (39) 02 90 78 19 05

B-K Medical (UK)
11 Grove Park
Waltham Road, White Waltham
Berkshire SL6 3LW
United Kingdom
Tel.: (44) 1628 825-770
Fax: (44) 1628 826 970

B-K Medical AB
Mänskärsvangen p
141 75 KUNGENS KURVA
Sweden
Tel.: (46) 8-744 02 11
Fax: (46) 8-744 02 12

**Your local distributor**